



HUMAC[®] NORM[®]

TESTING & REHABILITATION SYSTEM

*Measure & Improve
Performance*



Unparalleled Software and Mechanical Design

CSMi is proud to introduce the new HUMAC NORM Testing & Rehabilitation System. With the acquisition of CYBEX Medical, CSMi is now able to offer in one machine the industry-leading HUMAC Software coupled with the proven mechanical design of the CYBEX NORM.




CSMi has earned a worldwide reputation as an industry innovator and provider of quality, customer oriented products. I am pleased the CYBEX Medical products are now under their stewardship.

Dave Hillery
 President of CYBEX Division of Lumex
 1970-1990

Table of Contents


History	2-3
Solutions	4-5
Defined	6-7
Patterns	8-9
Options	10-11

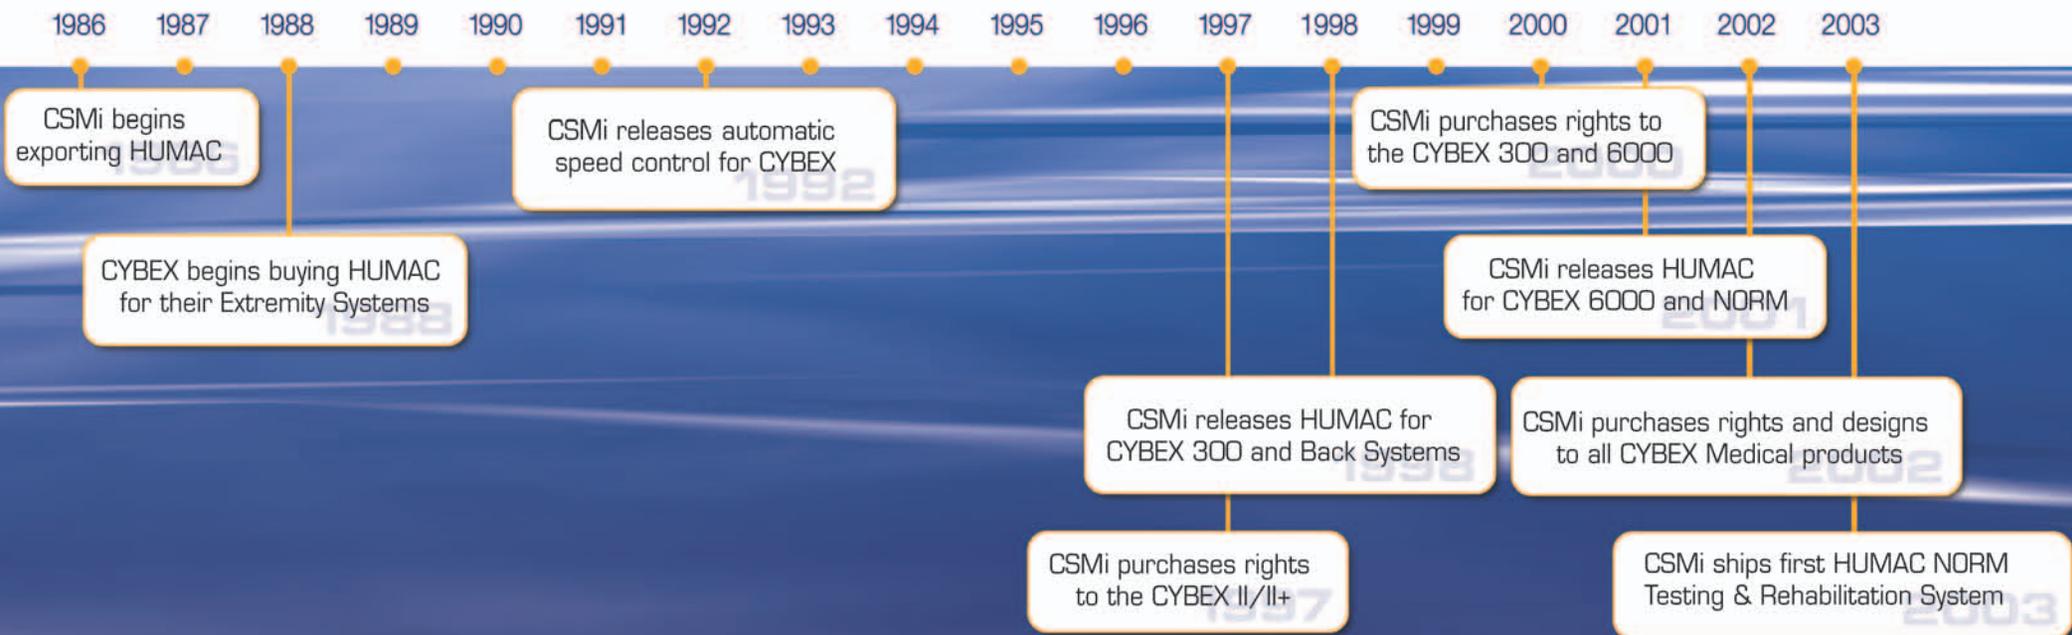

HUMAC[®] NORM[®] Solutions

TESTING & REHABILITATION SYSTEM

The HUMAC NORM is your solution for measuring and improving human performance in the clinic, training room, and research laboratory. In one machine the HUMAC NORM offers 22 isolated-joint movement patterns, four resistance modes (isokinetic, isotonic, isometric, and passive) and numerous reports to meet the measurement and exercise needs of today's clinicians and researchers.

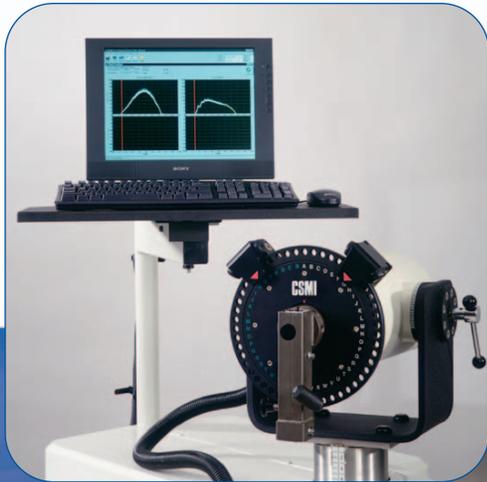

Measurement

Only with testing can you determine baselines, set goals, and track change. The HUMAC NORM offers two primary measurement solutions.

- **Isometric Testing:** when dynamic movement is a concern, isometric testing is the answer. The HUMAC NORM will safely position the patient to each angle in the protocol. Protocol options include angles, hold-times, rest periods, repetitions, and sets.
- **Isokinetic Testing:** to determine maximum dynamic capability throughout the range-of-motion isokinetic testing is the solution. The HUMAC NORM offers concentric and eccentric resistance testing. Isokinetic curve results make it easy determine areas of pain or weakness and determine capability.

Exercise

Exercise is performed to improve mobility, stability, strength, and control. The HUMAC NORM offers four modes of resistance and numerous feedback options to meet these goals.

- **Passive Mode:** develop the mobility that the patient requires, from straight pattern movements to complex PNF patterns.
- **Isometric Mode:** stabilize the joint to perform angle-specific strength training.
- **Isokinetic Mode:** continue to strengthen using proven methods to enhance return-to-function including concentric and eccentric loading and deceleration training.
- **Isotonic Mode:** complete the return-to-function training using our simulated mass isotonic mode.



The HUMAC NORM Testing & Rehabilitation System is the one machine that fulfills the testing and exercise needs of today's clinicians and researchers. The HUMAC Software makes it easy to operate.

Software

The HUMAC Software was designed with one goal in mind – enable the user to go from patient setup to report in hand as quickly as possible. Time is a limited commodity in every setting. This is why we chose Windows XP styling for the HUMAC Software. It is immediately recognizable to all users, so learning and operating the HUMAC NORM is a snap.

Intuitive Steps

To perform a test or exercise simply select patient, pattern, protocol and you are ready to start the session. The next time the patient is on the HUMAC NORM the process is even faster. Select QuickTest or QuickEx to go directly from patient selection to session. The HUMAC automatically applies test or exercise protocol used from the most recent session.


Personalize Your Preferences

The HUMAC's Preference settings give you the flexibility to customize the software to your specific needs. Preference options include Feedback, Data Analysis, and Reporting.

Your Software is never obsolete

CSMi continues to develop the HUMAC Software. And we always make sure the HUMAC Software is backwards compatible with all of our machines. From the earliest CYBEX II to the latest HUMAC NORM, your investment is never obsolete.

Visit www.csmisolutions.com to see sample HUMAC screens.

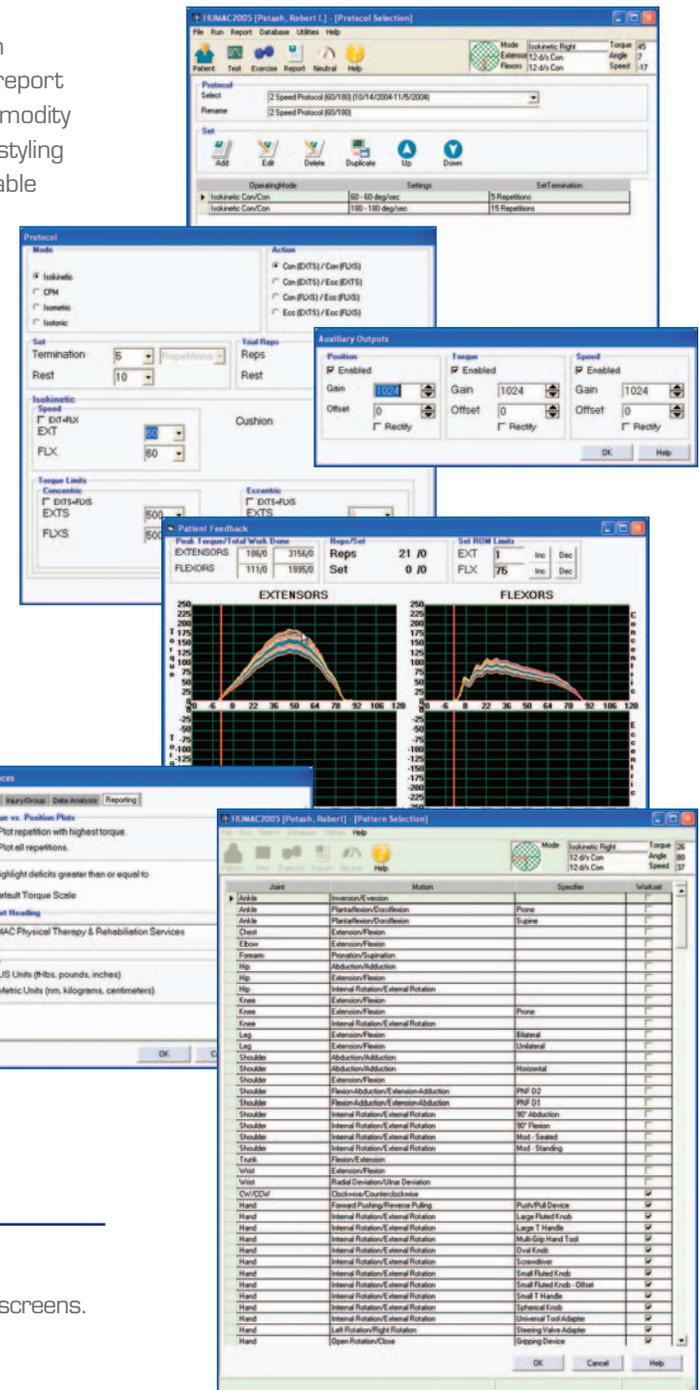

HUMAC[®] NORM[®]

TESTING & REHABILITATION SYSTEM

Defined

SECURE PATIENT POSITIONING

The HUMAC NORM seat area is 1,220 square inches. The large seat, coupled with fore/aft seat back positioning and a four point seatbelt harness, accommodates and stabilizes small and big, young and old patients alike.

MOVABLE CHAIR - FIXED DYNAMOMETER

The patented dynamometer/seat configuration minimizes floor space and adjustments, and insures quick and secure patient set-ups.

LOCKING CLAMPS

The locking clamps secure the dynamometer and seat in place. This design offers infinite positioning options and unmatched rigidity and durability. Dual clamps allow adjustments from either side of the machine.

CONTINUOUS ROTATION

The dynashaft allows continuous 360° rotation to simulate work patterns such as turning a wheel or screwdriver.

ADJUSTABLE RANGE-OF-MOTION STOPS

With the Adjustable Range-of-Motion Stops you do not have to change adapters each time you change sides.

MAXIMUM RESISTANCE

The HUMAC NORM dynamometer offers 500 ft-lbs. of eccentric and concentric force.



INTUITIVE USER INTERFACE

Our easy-to-use HUMAC software creates a machine everyone can operate.

CONTEXT-SENSITIVE HELP SYSTEM

Each HUMAC NORM window includes a Help button. Simply press Help and the on-line Help System opens to the very page you are on in the software.

INTEGRATED COMPUTER SYSTEM

The integrated computer system design saves floor space, reduces cables, and guarantees the keyboard and monitor will always be within reach.

AUXILIARY OUTPUTS (AO)

The auxiliary outputs provide easy access to torque, position, and velocity analog signals for input into other systems such as EMG. Our AO Software Control Window lets you adjust the Gain and Offset and rectify the signals to your requirements.

HUMAC Reports

The HUMAC offers a variety of easy-to-read, easy-to-interpret reports. Full-page reports are in color and can be printed, previewed, or e-mailed. Raw data is automatically saved for export to Excel or other formats.

HUMAC Reports Options Include:

- Test
- Curve Overlay
- Graphic Summary
- Exercise
- Narrative
- Repeatability
- Progress
- Group Summary
- Multi-Session
- Normative Data

Default Deficits & Exploded view

Deficits are automatically highlighted if they exceed the default value. Individual repetition values can be seen by clicking Zoom while previewing a test.




Preference Override

The HUMAC Report Preferences such as average vs. best rep; default deficit values; metric vs. US units, are applied to every report. Preference Override lets you change any setting immediately before printing a report.

Normative Data 20,000 Tests Strong

The HUMAC includes a database of 20,000 normal Knee and Shoulder test results. This allows you to compare your test results to one of the largest isokinetic normative data databases in the world.

Visit www.csmisolutions.com to see sample HUMAC Reports.

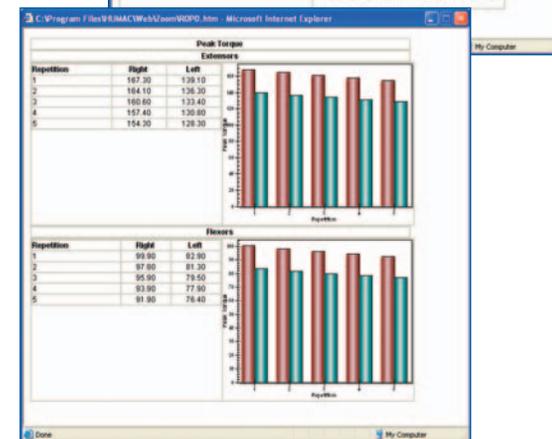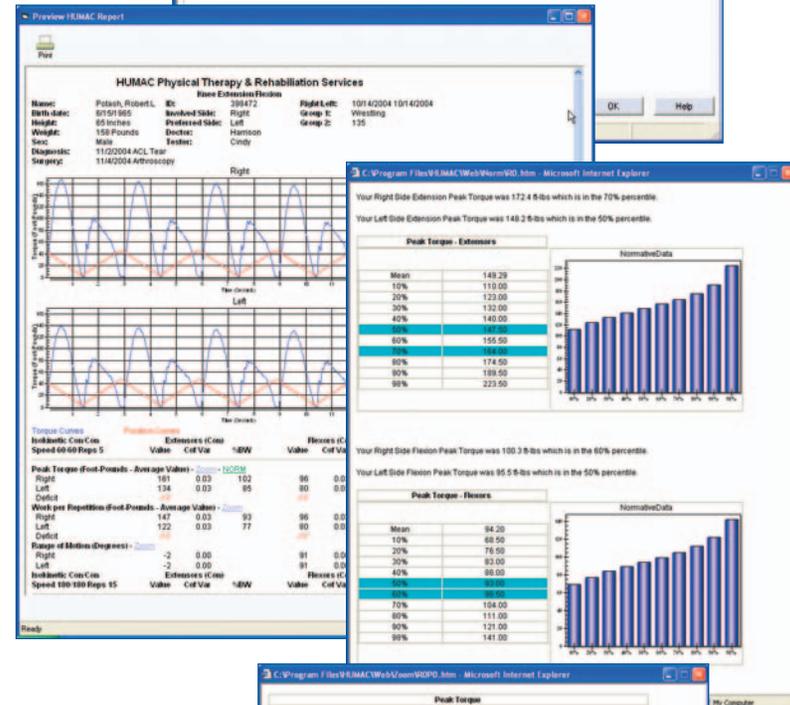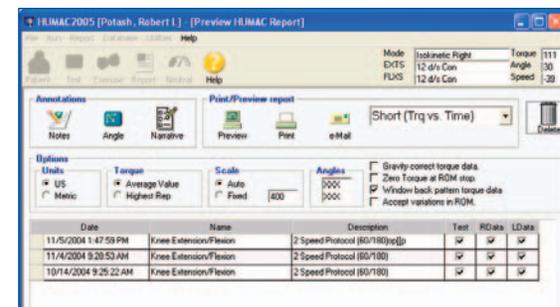


HUMAC[®] NORM^{ack}

TESTING & REHABILITATION SYSTEM

The HUMAC NORM includes attachments to perform 22 isolated patterns covering the shoulder, elbow, wrist, hip, knee, ankle and back. Optional attachments allow trunk extension/flexion, work simulation, and closed kinetic chain patterns.

Knee: Extension/Flexion Seated

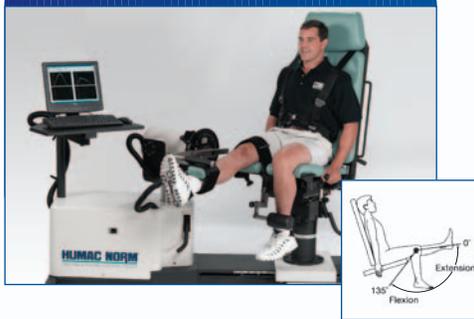

Knee: Extension/Flexion Prone



Knee: Tibial Internal/External Rotation



Shoulder: Extension/Flexion



Shoulder: Horizontal Abduction/Adduction




Shoulder: Internal/External Rotation in 90° Abduction




Shoulder: Internal/External Rotation, Mod-Standing



Forearm: Pronation/Supination

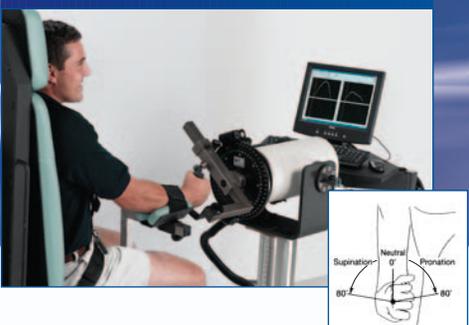

Wrist: Extension/Flexion

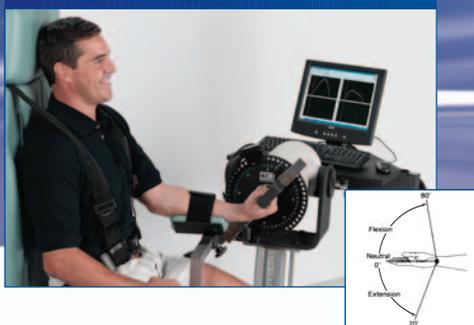


Wrist: Radial/Ulnar Deviation




Elbow: Extension/Flexion




Ankle: Plantar/Dorsiflexion Prone




Ankle: Plantar/Dorsiflexion Supine




Ankle: Inversion/Eversion




Shoulder: Abduction/Adduction




Shoulder: Internal/External Rotation, Mod-Seated




Shoulder: Internal/External Rotation in 90° Flexion




PNF D1: Flexion-Adduction/Extension-Abduction




PNF D2: Flexion-Abduction/Extension-Adduction




Hip: Abduction/Adduction




Hip: Flexion/Extension



Hip: Internal/External Rotation



Trunk: Flexion/Extension



Trunk Modular Component (TMC)

With the TMC the HUMAC NORM is perfectly suited for trunk testing and rehabilitation in a fully functional, standing position. The motorized footplate ensures accurate patient positioning. The low inertia input assembly and lightweight attachment enables patients to begin rehabilitation sooner.

Johnson Anti-Shear™ Accessory

The Johnson Anti-Shear Dual Pad Accessory with adjustable fulcrum allows the clinician to select the correct amount of counterforce necessary to control anterior shear during knee extension. This prevents excessive stress on repairs, healing, or chronically lax ligaments.

Work Simulation Package

The Work Simulation Package allows clinicians to simulate an unlimited number of real-life and occupational patterns. The attachments include an assortment of handles and knobs, a steering device, a gripping device, and a push/pull device. Because the HUMAC NORM's dynamometer shaft allows full 360° rotation you enjoy a greater range of exercise options.

Closed Kinetic Chain (CKC) Accessory

The CKC expands the HUMAC NORM from a rotary device to a linear device. Use the rugged CKC to test and exercise patients in linear, closed chain patterns. The CKC includes attachments to perform a single and bilateral leg press, and bilateral chest press.

COLOR COORDINATED

The HUMAC NORM standard colors include a white plastic shroud and a black frame with teal upholstery. If your color needs are different we invite you to select the color shroud (white or black), frame, and upholstery that match your facility. We can embroider your logo into the seat back. Custom colors and embroidery requests slightly increase final price and delivery time.



Trunk Modular Component (TMC)



Johnson Anti-Shear™ Accessory



Work Simulation Package



Closed Kinetic Chain (CKC) Accessory

Resistance Modes

Mode

Isokinetic Concentric
Isokinetic Eccentric
CPM
Isometric
Isotonic


Speeds

$\frac{1}{16}$ - 500^o per sec
 $\frac{1}{16}$ - 300^o per sec
 $\frac{1}{16}$ - 150^o per sec

Torque

500 ft-lbs/678 Nm
500 ft-lbs/678 Nm
150 ft-lbs/203 Nm
500 ft-lbs/678 Nm
500 ft-lbs/678 Nm

Suggested floor plan

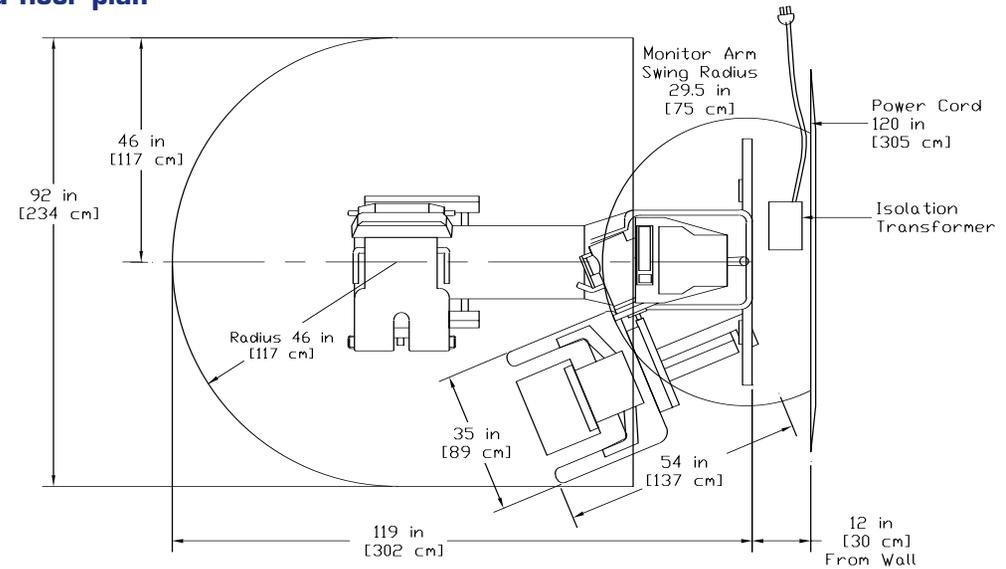


Electrical Specifications

Independent 20 Amp single phase line. Can be configured for input voltages between 184 and 259 VAC. Shipped configured for 208 VAC. Recommended outlet receptacle NEMA 6-20R (Hospital Grade)

Power Requirements


Input Voltage: 220 VAC (other voltages available)
Input Frequency: 60Hz (international frequency 50Hz available)
Independent 20 amp dedicated circuit required

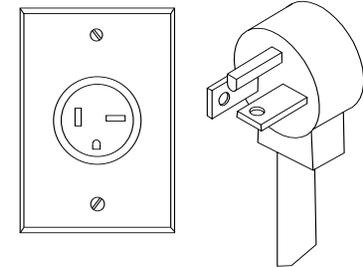

Black shroud w/ gray frame.




White shroud w/ black frame.



Upholstery is available in color combinations to match your team or facility.

Visit www.csmisolutions.com to learn more about HUMAC options.

- PT Clinic Website Design Tool
- PVI Home Exercise Software
- SportsWare™ Injury Tracking Software
- HUMAC Computer System Upgrade for CYBEX Extremity Systems
- Service and Support for CYBEX II/II+, 300 Series, Back Series, 6000, and NORM
- New HUMAC NORM Single Chair Extremity System
- Balance System
- Kinetron Lower Extremity Rehabilitation System

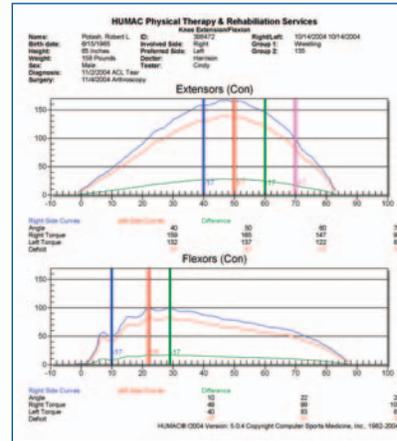

HUMAC Physical Therapy & Rehabilitation

Monday, November 15, 2004

Report on: Patient, Robert L.

Dear Dr. Harmon:

Thank you for referring Robert Potash for HUMAC/NORM isometric testing. The Patient has a diagnosis of ACL Tear.

The following graphs show the force curves of the Right vs. the Left superimposed, showing a comparative picture of the individual's ability to produce force throughout the ROM.

In normal subjects, imbalances of 10% or less can be considered normal while differences of 10% to 20% possibly abnormal and those 20% and above probably abnormal. * The patient produced the following results:

Muscle	Right	Left	Deficit
Extensors	107.00	134.00	-17%
Flexors	56.00	80.00	-17%

The patient would benefit from physical therapy to improve strength. My treatment plan will include isolated and functional strength training. If you have any comments or suggestions concerning the patient, contact me directly at 781-297-2034.

Sincerely,
 Richard Collins

* Muscle Performance Evaluation in Orthopaedic Practice, Alexander A. Swegart, MD, Journal of Bone and Joint Surgery, Vol 72A, New 10, Dec 1990

www.csmisolutions.com info@csmisolutions.com
 101 Tosca Drive Stoughton, MA 02072 Voice: (781) 297-2034 FAX: (781) 297-2039

HUMAC Physical Therapy & Rehabilitation Services
Knee Extensors/Flexors

Name: Patient, Robert L. ID: 30472
 Birth date: 07/17/1955 Injured Site: Right Right Leg: 10/14/2004 10/14/2004
 Height: 65 inches Preferred Side: Left Group 1: Walking Group 2: 150
 Weight: 158 Pounds Doctor: Harmon
 Sex: Male Tester: Only
 Diagnosis: 11022004 ACL Tear
 Surgery: 11022004 Arthroscopy

Extensors (Con)

Substrate	Cardiac	Speed	Reps	10/14/2004	11/14/2004	Change	10/14/2004	11/14/2004	Change
Peak Torque (Peak Pounds - Average Value)	Right	179	18	86	108	10	108	10	0
Left	157	23	80	88	14				
Deficit									
Work per Repetition (Peak Pounds - Average Value)	Right	103	18	86	107	11	107	11	0
Left	122	22	80	88	14				
Deficit									
Change of Motion (Degrees)	Right	-2	-11	0	0	0	0	0	0
Left	-2	-11	0	0	0	0	0	0	0
Deficit									
Range of Motion (Degrees)	Right	-2	-11	0	0	0	0	0	0
Left	-2	-11	0	0	0	0	0	0	0
Deficit									

Flexors (Con)

Substrate	Cardiac	Speed	Reps	10/14/2004	11/14/2004	Change	10/14/2004	11/14/2004	Change
Peak Torque (Peak Pounds - Average Value)	Right	102	18	88	100	11	100	11	0
Left	158	24	81	88	15				
Deficit									
Work per Repetition (Peak Pounds)	Right	196	217	202	1300	1400	1400	1400	140
Left	187	1949	282	1084	1275	191	1275	191	0
Deficit									
Change of Motion (Degrees)	Right	-2	-11	0	0	0	0	0	0
Left	-2	-11	0	0	0	0	0	0	0
Deficit									

HUMAC® (2004) Version: 5.0.4 Copyright Computer Sports Medicine, Inc. 1983-2004